


Small & Large NiMH Battery Packs

REF 7505-710 and REF 6640-710

Instructions for Use

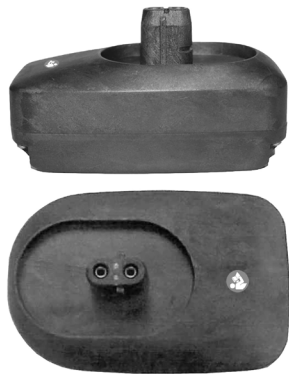

MICROAIRE®
For Surgery. For Life.™

Battery Replacement

Over time and with repeated use, the physical characteristics of the REF 7505-710 and REF 6640-710 Battery Packs may be diminished. Replacement of the battery should be considered if:

- The Battery Pack shows signs of physical damage, including cracks and loose or missing parts.
- The gold-plated terminals show sign of corrosion and wear.
- The Battery Pack shows significantly reduced run-time or insufficient power when used with MicroAire instruments.
- Instruments such as the oscillating saw suddenly start to stall when heavily loaded.
- The "Charge Failed" light on the 7500-700 charger comes on repeatedly.

MARKINGS

Symbol	Definition
	This icon is blue. Follow Instructions for Use.
	Indicates the European Conformity Mark with Notified Body Number. 2797 is the BSI-NL-registered Notified Body.
	Do not immerse
	Product catalog number
	Product serial number
	Temperature Limitation

INDICATIONS FOR USE

The MicroAire REF 7505-710 Large Battery Pack and REF 6640-710 Small Battery Pack are intended for use with MicroAire U.L. classified Battery Powered Instruments and Chargers. A list of compatible devices is presented below:

COMPATIBLE DEVICES FOR REF 7505-710

Product Catalog Number	Description
REF 6643/REF 6642B*	Battery SmartDriver Duo™
REF 7505/REF 7500*	Drill/Reamer
REF 7506/REF 7600*	Oscillating Saw
REF 7507/REF 7700*	Reciprocating Saw
REF 7800	Sternum Saw
REF 7500-700	MicroAire Battery Charger

COMPATIBLE DEVICES FOR REF 6640-710

Product Catalog Number	Description
REF 6643/REF 6642B*	Battery SmartDriver Duo™
REF 7800	Sternum Saw
REF 7500-700	MicroAire Battery Charger

- NOTE:** Used to point out the easiest Means of carrying out techniques.
- CAUTION:** Used to point out special procedures or precautions that must be followed to avoid damaging the systems.
- WARNING:** Used to indicate that the safety of the patient and hospital personnel could be involved.

MARKINGS (CONTINUED)

Symbol	Definition
	European authorized representative
	Humidity Limitation
	Atmospheric Pressure Limitation
	Waste Electrical and Electronic Equipment (WEEE) European Community Symbol. Batteries contain materials that must be recycled or disposed of properly. Do not dispose of as unsorted municipal waste. ALWAYS follow the current local recommendations and/or regulations governing environmental protection and the risks associated with recycling or disposing of the equipment at the end of its usual life. ALWAYS decontaminate a battery pack exposed to infectious material before sending it to a waste treatment facility.
	Date of manufacture. Y=year, M=month.
	Manufacturer
	Prescription

CLEANING AND STERILIZATION

Cleaning

1. Wipe external surfaces of the battery with a disinfectant after each procedure and rinse under warm water.
2. Dry with a lint-free cloth.

CAUTION: The REF 7505-710 and REF 6640-710 Battery Packs are NOT IMMERSIBLE.

ENVIRONMENTAL CONDITIONS

	Operation	Storage and Transportation
Temperature limits	32°F/0°C 86°F/30°C	0°F/-20°C 120°F/49°C
Relative humidity limits	0% 91%	0% 91%
Atmospheric pressure limits	70 -106 kPa	70 -106 kPa

- NOTE:** Always follow the current local recommendations and/or regulated governing environmental protection and the risks associated with recycling or disposing of the equipment at the end of its useful life.
- NOTE:** Always decontaminate a battery pack expose to infectious material before sending it to a waste treatment facility.
- WARNING:** Use ONLY with U.L. Classified MicroAire Battery Powered Instruments.
- WARNING:** No modification of this equipment is allowed.
- WARNING:** Operating Duty cycle for REF 6643 and REF 7500 is 1 minute on, 1 minute off for a maximum of 6 cycles. Operating Duty cycle for REF 7800 is 1 minute on, 2 hours off.
- CAUTION:** Federal Law restricts this device to sale by or on the order of a physician (or properly licensed practitioner).
- *NOTE:** Instruments REF 6642B, REF 7500, REF 7600, and REF 7000 are compliant to UL 60601-1/IEC 60601-1:2nd edition only.

Sterilization

The following sterilization processes have been validated based on AAMI protocols. The exposure times and temperatures are the minimum validated requirements to ensure sterility. Gravity displacement is the preferred method for battery sterilization.

Gravity Displacement Steam

- 3 minutes @ 270° F - 279° F (132° C - 137° C), unwrapped
- No drying time

CAUTION: A five-minute gravity cycle is acceptable if a pre-programmed autoclave only has one cycle.

Dynamic Air Removal (Pre-vacuum)

- 4 minutes @ 270° F - 279° F (132° C - 137° C), wrapped or unwrapped
- No drying time

Sterrad® 100 Sterilization

- 44 minutes total exposure time

Sterrad® NX Sterilization

- 28 minutes full cycle

WARRANTY

MicroAire Surgical Instruments warrants the REF 7505-710 Large Battery Pack and REF 6640-710 Small Battery Pack to be free from defects in material and workmanship in their manufacture for a period of one (1) year from the original purchase date by the end customer. The warranty is limited to the repair or replacement of the product without charge.

This warranty is void in the event of abuse, misuse, or use in other than normal surgical environment, or in the event of disassembly, alteration or the repair of the product not

SET UP

- NOTE:** Clinical personnel should become familiar with the Battery Pack before it is set up for use in any procedure.
- NOTE:** For best results, the Battery Pack should be fully charged prior to use.
- CAUTION:** Prior to and after use, inspect for cracks, loose or missing parts, or other damage. Such defects can affect product performance.

To attach the battery pack to a MicroAire Battery Powered Instrument, refer to the applicable instrument instruction manual:

- To attach the battery pack to a MicroAire REF 7505, REF 7506, or REF 7507 Battery Powered Instrument, refer to IM-7505.
- To attach the battery pack to the MicroAire REF 6643 SmartDriver Duo™, refer to IM-6643.
- To attach the battery pack to the MicroAire REF 7800 Sternum Saw, refer to IM-7800.

BATTERY CARE

Battery Charging

- WARNING:** Do not charge in the patient vicinity.
- CAUTION:** MicroAire REF 7505-710 Large Battery Packs and REF 6640-710 Small Battery Packs should only be charged using the MicroAire REF 7500-700 MicroAire Battery Charger.

To charge the battery pack, refer to the operating instructions for the MicroAire REF 7500-700 MicroAire Battery Charger in manual IM-7500-700.

WARRANTY (CONTINUED)

authorized by the manufacturer, or in the event that the product has not been used in a reasonable manner, and in compliance with the written instructions furnished by the manufacturer.

All other expressed or implied warranties of fitness and merchantability are excluded here from and manufacturer shall have no liability of any kind for incidental or consequential damages.

Due to the nature of batteries, extended warranties are not available for the battery pack.

REPAIR SERVICE

If a problem with your equipment should arise, contact our Customer Service Department at:

	Telephone	Fax	Email
USA	800-722-0822	800-438-6309	inquiry@microaire.com
Outside USA	434-975-8000	434-975-4134	intlsvcs@microaire.com



MicroAire Surgical Instruments, LLC
3590 Grand Forks Boulevard
Charlottesville, Virginia 22911 USA
Phone: (800) 722-0822 (434) 975-8000
Order Fax: (800) 648-4309 or (434) 975-4131
www.microaire.com



MediMark Europe
11, rue Emile Zola -
BP 2332
F-38033 Grenoble
Cedex 2
France